

Integrating the Healthcare Enterprise



5

**IHE Radiation Oncology  
Technical Framework Supplement**

10

**Multimodality Image Registration for Radiation  
Oncology 2013  
(MMRO – III)**

15

**Rev. 1.1 – Trial Implementation**

20

Date: November 16, 2016  
Author: IHE Radiation Oncology Technical Committee  
Email: ro@ihe.net

25

**Please verify you have the most recent version of this document. See [here](#) for Trial Implementation and Final Text versions and [here](#) for Public Comment versions.**

## Foreword

30 This is a supplement to the IHE Radiation Oncology Technical Framework V1.8. Each supplement undergoes a process of public comment and trial implementation before being incorporated into the volumes of the Technical Frameworks.

This supplement is published on November 16, 2016 for trial implementation and may be available for testing at subsequent IHE Connectathons. The supplement may be amended based on the results of testing. Following successful testing it will be incorporated into the Radiation Oncology Technical Framework. Comments are invited and can be submitted at  
35 [http://www.ihe.net/Radiation\\_Oncology\\_Public\\_Comments](http://www.ihe.net/Radiation_Oncology_Public_Comments).

NOTE: This supplement defines an update to the IHE-RO MMRO-II Profile originally developed in 2012. It relaxes some of the requirements that were put on the direction of registrations and modalities involved.

This supplement describes changes to the existing technical framework documents.

40 “Boxed” instructions like the sample below indicate to the Volume Editor how to integrate the relevant section(s) into the relevant Technical Framework volume.

<i>Amend Section X.X by the following:</i>
--

45 Where the amendment adds text, make the added text **bold underline**. Where the amendment removes text, make the removed text **~~bold strikethrough~~**. When entire new sections are added, introduce with editor’s instructions to “add new text” or similar, which for readability are not bolded or underlined.

General information about IHE can be found at: [www.ihe.net](http://www.ihe.net).

Information about the IHE Radiation Oncology domain can be found at: [ihe.net/IHE\\_Domains](http://ihe.net/IHE_Domains).

50 Information about the organization of IHE Technical Frameworks and Supplements and the process used to create them can be found at: [http://ihe.net/IHE\\_Process](http://ihe.net/IHE_Process) and <http://ihe.net/Profiles>.

The current version of the IHE Radiation Oncology Technical Framework can be found at: [http://ihe.net/Technical\\_Frameworks](http://ihe.net/Technical_Frameworks).

55

60

## CONTENTS

65	Introduction to this Supplement.....	5
	Open Issues and Questions .....	5
	Closed Issues .....	5
	<b>Volume 1 – Profiles .....</b>	<b>7</b>
	1.7 History of Annual Changes.....	7
70	1.9 Copyright Permission.....	7
	2.1 Dependencies among Integration Profiles .....	7
	2.2.X Multimodality Image Registration for Radiation Oncology 2013 Integration Profile	8
4	Multimodality Image Registration for Radiation Oncology 2013 (MMRO-III) Profile .....	9
	4.1 MMRO-III Actors, Transactions, and Content Modules .....	9
75	4.1.1 Actor Descriptions and Actor Profile Requirements .....	11
	4.2 MMRO-III Actor Options.....	12
	4.3 MMRO-III Actor Required Groupings.....	13
	4.4 MMRO-III Document Content Module.....	14
	4.5 MMRO-III Overview .....	14
80	4.5.1 Concepts .....	14
	4.5.2 Use Case #1: Multimodality Contouring .....	18
	4.5.3 Use Case #2: Shared Frame of Reference .....	20
	4.5.4 Use Case #3: Multimodality Dose Display .....	22
	4.6 MMRO-III Security Considerations .....	23
85	4.7 MMRO-III Cross Profile Considerations.....	23
	Appendices.....	24
	Actor Summary Definitions .....	24
	Transaction Summary Definitions .....	24
	Glossary .....	25
90	<b>Volume 2 – Transactions.....</b>	<b>26</b>
	3 Transactions .....	27
	3.14MMRO-3: Registered Structure Set Storage .....	27
	3.14.1 Scope .....	27
	3.14.2 Use Case Roles .....	27
95	3.14.3 Referenced standards.....	27
	3.14.4 Interaction Diagram.....	28
	3.14.5 Security Considerations.....	29
	3.15MMRO-4: Registered Structure Set Retrieval .....	29
	3.15.1 Scope .....	29
100	3.15.2 Use Case Roles .....	29
	3.15.3 Referenced standards.....	30
	3.15.4 Interaction Diagram.....	30
	3.15.5 Security Considerations.....	31

	3.16MMRO-5: Registered Dose Retrieval .....	31
105	3.16.1 Scope .....	31
	3.16.2 Use Case Roles .....	32
	3.16.3 Referenced Standards .....	32
	3.16.4 Interaction Diagram .....	32
	3.16.5 Security Considerations .....	33
110	3.17MMRO-III-1: Spatial Registration-III Storage .....	33
	3.17.1 Scope .....	33
	3.17.2 Use Case Roles .....	34
	3.17.3 Referenced Standards .....	34
	3.17.4 Interaction Diagram .....	34
115	3.17.5 Security Considerations .....	36
	3.18MMRO-III-2: Spatial Registration-III Retrieval .....	36
	3.18.1 Scope .....	36
	3.18.2 Use Case Roles .....	36
	3.18.3 Referenced Standards .....	37
120	3.18.4 Interaction Diagram .....	37
	3.18.5 Security Considerations .....	38
	Appendix A – Attribute Consistency between Composite IODs .....	39
	A.1 Radiation Oncology Critical Attribute Mapping .....	39
	A.2 Radiation Oncology Critical Modules .....	39
125	A.3 Radiation Oncology Critical Attributes .....	40

## Introduction to this Supplement

130 This supplement defines the Multimodality Image Registration for Radiation Oncology 2013 Profile (MMRO-III). It adds information to Volumes 1 and 2 and of the IHE Radiation Oncology Technical Frameworks to describe the profile and define the actors and transactions that are present in the profile.

135 The Multimodality Image Registration for Radiation Oncology 2013 Profile specifies communications between systems creating and registering image sets. It defines how DICOM®<sup>1</sup> objects for spatial registration and the images themselves are created, stored, queried, retrieved, processed and displayed.

This document resembles the base definition from MMRO and the changes that were performed for MMRO-II.

## Open Issues and Questions

#	Intr. in	Description
1	Prepub 1.5	Should systems be able to handle non-orthogonal orientations for RT Dose? As primary? As secondary? Affine vs. non-affine. TC 20141014: Open issue for Public Comment: vendors to find out what is supported e.g., in case of planning on an MR: pure orthogonal dose planes or planes in the orientation of the MR

## Closed Issues

#	Intr. in	Description
2	Prepub 1.5	Removed requirement for a "primary" FOR being the FOR of a CT image series. By this, allowing chained registrations and no more "stars".
3	Prepub 1.5	Deformable Registration will be handled in a separate profile (from TC on Feb 21, 2013)
4	Prepub 1.5	Patient repositioning is NOT a use case of this profile.
5	Prepub 1.5	Only 2 FORs will be registered with one Registration object. There shall be 2 items in the registration sequence of the object. Each FOR must be distinct; the FORs listed in the sequence cannot be identical.
6	Prepub 1.5	The identity matrix must be present for one of the sequence items.
7	Prepub 1.5	Actor names can stay "as is". Actors are referenced by the profile they appear under.
8	Prepub 1.5	What are the implications of additional use cases involving 4D imaging and image guidance acquisition? 4D imaging does not cause issues in rigid registration workflow. In general, 4D challenges are in the area of segmentation as you have structure tracking across the time sequence of images. For registration, deformable registration is the process used in 4d, and that will be covered in a different profile.
9	Prepub 1.5	Mention the behavior for a Well-known FOR. Add a note that Well Known FOR usage is not addressed in this profile.

---

<sup>1</sup> DICOM is the registered trademark of the National Electrical Manufacturers Association for its standards publications relating to digital communications of medical information.

---

IHE Radiation Oncology Technical Framework Supplement – Multimodality Image Registration for Radiation Oncology 2013 (MMRO-III)

#	Intr. in	Description
10	Prepub 1.5	The RT Structure Set created on a registered image sets in this profile is limited to reference only to a single image set. In cases where multiple image sets have been registered to the referenced image set with different registrations, the Registered Display is not able to determine if the contours displayed to the user have been created on the image set combination currently displayed. This restriction was originally imposed to allow BRTO actors to use the objects created. Add note that determination is currently not possible under the DICOM 2011 standards.
11	Prepub 1.5	Discuss whether Registration Input Information (Fiducials, Segmentations) shall be part of this profile? Optional? TC 20141014: Not in current scope of this profile. Adding an open issue to DPDW Profile instead. 20141201: Moved to Closed Issues and sent a note to the author of DPDW.
12	Prepub 1.5	Is there a limit on the dis-orientation that is allowed? E.g., should registration of sagittal images with axial images be mandatory, or perhaps in a range (e.g., +/- 30 degrees)? TC 20141014: not an issue. Closed.
13	Prepub 1.5	Should drawing be required on the original secondary images, rather than those images re-sampled to the primary FoR? Projection of sagittal contours to an axial view TC 20141014: The profile enables contouring on either image set. Therefore, this is not an issue of the profile currently.
14	Prepub 1.5	Do we want to include a dose calculation actor in the profile? All current dose calculation actors require axial orientations of dose calculations. Should we allow non-orthogonal dose planes: Gyn applicator planes Calculations on MR planes for SRS systems. TC 20141014: Not the right time, should be addressed when the content and workflow profiles are written.
15	Prepub 1.5	Should RO-5 (Dose Retrieval) be replaced with a more modern one, so that dose can be stored in any of the FoRs present in an application (FoR of CT, MR, ...)? This would also allow updating of RO-5 to DICOM 2007, or we could CP BRTO to move it to DICOM 2011? TC 20141014: Decision to leave BRTO as is, updated MMRO-5 Registered Dose Retrieval accordingly.
16	Prepub 1.6	TC 20141014: Include MMRO and MMRO-II in the MMRO-III document to have again a single document to make it easier for the editor of the TF to understand what to include

140

## Volume 1 – Profiles

### 1.7 History of Annual Changes

Add the following to the IHE Technical Frameworks General Introduction Section 1.7:

- 145 • Added the Multimodality Image Registration for Radiation Oncology 2013 Profile. In this profile, a Registrator performs a rigid alignment of two image sets for the same patient and stores this information in an interoperable manner within a Spatial Registration IOD. The alignment information can then be used to render contours and dose distributions on the image set overlay or to contour additional structures.

### 1.9 Copyright Permission

150 Add the following to the IHE Technical Frameworks General Introduction Copyright section:

### 2.1 Dependencies among Integration Profiles

Add the following to Table 2-1

Integration Profile	Depends on	Dependency Type	Purpose
Multimodality Image Registration for Radiation Oncology 2013	Scheduled Workflow	Acquisition Modality Image Storage [RAD-8]	Modality Images (CT, MR, PT... ) will be stored in the archive in accordance with the referenced transaction
Multimodality Image Registration for Radiation Oncology 2013	Scheduled Workflow	Creator Images Stored [RAD-18]	Created Images (CT, MR, PT... ) will be stored in the archive in accordance with the referenced transaction
Multimodality Image Registration for Radiation Oncology 2013	Basic Radiation Therapy Objects	Dose Storage [RO-5]	RT Dose will be stored in the archive in accordance with the referenced transaction
Multimodality Image Registration for Radiation Oncology 2013	Multimodality Image Registration for Radiation Oncology	Registered Structure Set Storage [MMRO-3]	RT Structure Set will be stored to the archive in accordance with the referenced transaction
Multimodality Image Registration for Radiation Oncology 2013	Multimodality Image Registration for Radiation Oncology	Registered Structure Set Retrieval [MMRO-4]	Archive will store RT Structure Set in accordance with the referenced transaction
Multimodality Image Registration for Radiation Oncology 2013	Multimodality Image Registration for Radiation Oncology	Registered Dose Retrieval [MMRO-5]	Archive will store RT Dose in accordance with the referenced transaction

155

*Add the following section to Section 2.2*

**2.2.X Multimodality Image Registration for Radiation Oncology 2013 Integration Profile**

160 The Multimodality Image Registration for Radiation Oncology Integration 2013 Profile involves the flow of multimodality image data to a Registrator to perform a rigid image alignment. The image sets in combination with the resulting Spatial Registration IOD can be consumed by Registered Contourers to create new contours. Additionally, Registered Displays or Registered Dose Displays can use the registered image sets to visualize contours or dose.



## 4 Multimodality Image Registration for Radiation Oncology 2013 (MMRO-III) Profile

165

This Integration Profile specifies how images, RT Structure Sets, RT Doses, and associated spatial registration information can be exchanged, stored, processed and displayed. For a display workstation, it is essential that a workstation correctly identifies the corresponding image sets, matches data from single-slice and multi-slice datasets, matches coordinate systems, and performs spatial translations. The use of relevant DICOM objects (Spatial Registration) is clarified and constrained in order to avoid misinterpretation.

170

The Multimodality Image Registration for Radiation Oncology 2013 (MMRO-III) Profile focuses on content for image registration and does not define a registration workflow. Such workflow could be managed by using mechanisms described in the Post-Acquisition Workflow Integration Profile (see RAD TF-1:12).

175

The MMRO-III Profile currently only handles rigid registration. Deformable registration will be addressed in a separate Profile in the future.

The MMRO-III Profile does not specify the use of quantification methods for the image data that are created or displayed. In particular, interoperability for PET Standard Uptake Values (SUV) is considered a relevant future work item for IHE. Note that vendors may wish to provide SUV capability even though not required under this Profile.

180

The MMRO-III Profile has implicit limitations imposed by its dependency on the IHE-RO BRTO Profile. The most significant of these are listed here:

185

- Only the following patient orientations {HFS, HFP, FFS, FFP} shall be considered to be within the scope of this profile. Actors participating in this profile may be capable of handling additional orientations (decubitus), but such orientations will not be tested with this profile.

The limitation that a base image set shall be defined that is of modality CT does not exist anymore. This allows creation of registrations between any kinds of image modalities in an arbitrary order.

190

RT Dose shall be in the Registered Frame of Reference, e.g., in the same Frame of Reference as its referenced image set.


### 4.1 MMRO-III Actors, Transactions, and Content Modules

195

Figure 4.1-1 shows the actors directly involved in the MMRO-III Profile and the relevant transactions between them. If needed for context, other actors that may be indirectly involved due to their participation in other related profiles are shown in dotted lines. Actors which have a mandatory grouping are shown in conjoined boxes.

This profile uses the MMRO Registered Contourer, which must be compatible with RT Structure Set objects created by the BRTO Profile Contourer.

200

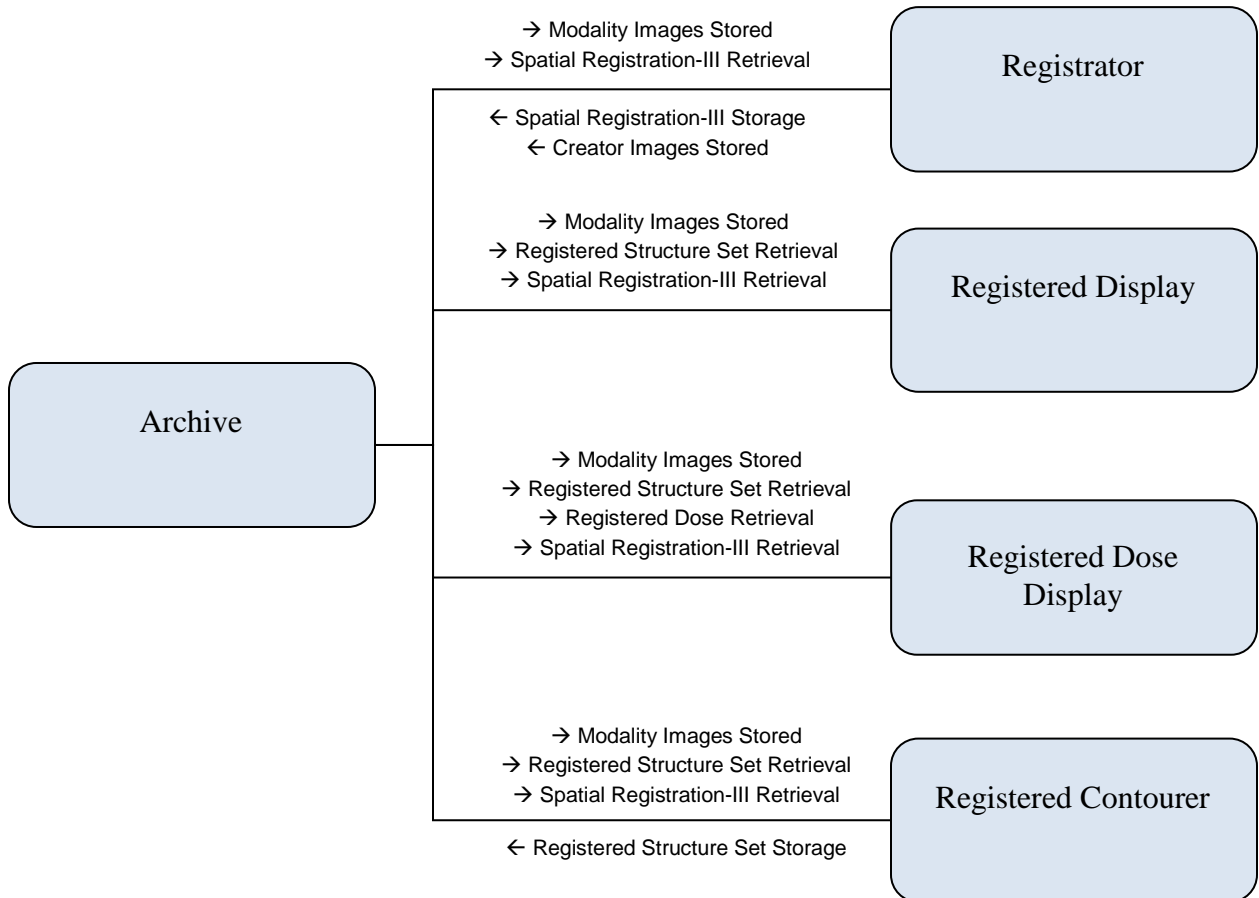

**Figure 4.1-1: MMRO-III Actor Diagram**

205 Table 4.1-1 lists the transactions for each actor directly involved in the MMRO-III Profile. In order to claim support of this Profile, an implementation of an actor must perform the required transactions (labeled “R”) and may support the optional transactions (labeled “O”). Actor groupings are further described in Section 4.3.

210

**Table 4.1-1: MMRO-III Profile - Actors and Transactions**

<b>Actors</b>	<b>Transactions</b>	<b>Optionality</b>	<b>Section in Vol. 2</b>
<b>Archive</b>	Modality Images Stored	R	RAD 4.8
	Creator Images Stored	R	RAD 4.18
	Registered Structure Set Storage	R	MMRO-3
	Spatial Registration-III Storage	R	MMRO-III-1
	Spatial Registration-III Retrieval	R	MMRO-III-2
	Registered Dose Retrieval	R	MMRO-5
	Registered Structure Set Retrieval	R	MMRO-4
<b>Registrar</b>	Modality Images Stored	R	RAD 4.8
	Creator Images Stored	O	RAD 4.18
	Spatial Registration-III Retrieval	O	MMRO-III-2
	Spatial Registration-III Storage	R	MMRO-III-1
<b>Registered Contourer</b>	Modality Images Stored	R	RAD 4.8
	Registered Structure Set Storage	R	MMRO-3
	Registered Structure Set Retrieval	R	MMRO-4
	Spatial Registration-III Retrieval	R	MMRO-III-2
<b>Registered Display</b>	Modality Images Stored	R	RAD 4.8
	Registered Structure Set Retrieval	R	MMRO-4
	Spatial Registration-III Retrieval	R	MMRO-III-2
<b>Registered Dose Display</b>	Modality Images Stored	R	RAD 4.8
	Registered Structure Set Retrieval	R	MMRO-4
	Registered Dose Retrieval	R	MMRO-5
	Spatial Registration-III Retrieval	R	MMRO-III-2

#### 4.1.1 Actor Descriptions and Actor Profile Requirements

No special requirements

## 4.2 MMRO-III Actor Options

215 Options that may be selected for this Profile are listed in the Table 4.2-1 along with the actors to which they apply. Dependencies between options when applicable are specified in notes.

**Table 4.2-1: MMRO-III - Actors and Options**

<b>Actor</b>	<b>Options</b>	<b>Volume &amp; Section</b>
Archive	<i>No options defined</i>	--
Registrator	<i>Creator Images Stored</i>	RAD 4.18
	<i>Spatial Registration-III Retrieval</i>	MMRO-III-2
Registered Contourer	<i>No options defined</i>	--
Registered Display	<i>No options defined</i>	--
Registered Dose Display	<i>No options defined</i>	--

220 **4.3 MMRO-III Actor Required Groupings**

Actor(s) which are required to be grouped with another actor(s) are listed in this section. The grouped actor may be from this profile or a different domain/profile. These mandatory required groupings, plus further descriptions if necessary, are given in the table below.


225 An actor from this profile (Column 1) must implement all of the required transactions in this profile in addition to all of the required transactions for the grouped profile/actor listed (Column 2).

**Table 4.3-1: MMRO-III - Actors Required Groups**

<b>MMRO Actor</b>	<b>Required Grouping Actor</b>	<b>Technical Framework Reference</b>	<b>Note</b>
Archive	None	--	
Registrar	None	--	
Registered Contourer	None	--	
Registered Display	None	--	
Registered Dose Display	None	--	

## 4.4 MMRO-III Document Content Module

### 230 4.5 MMRO-III Overview

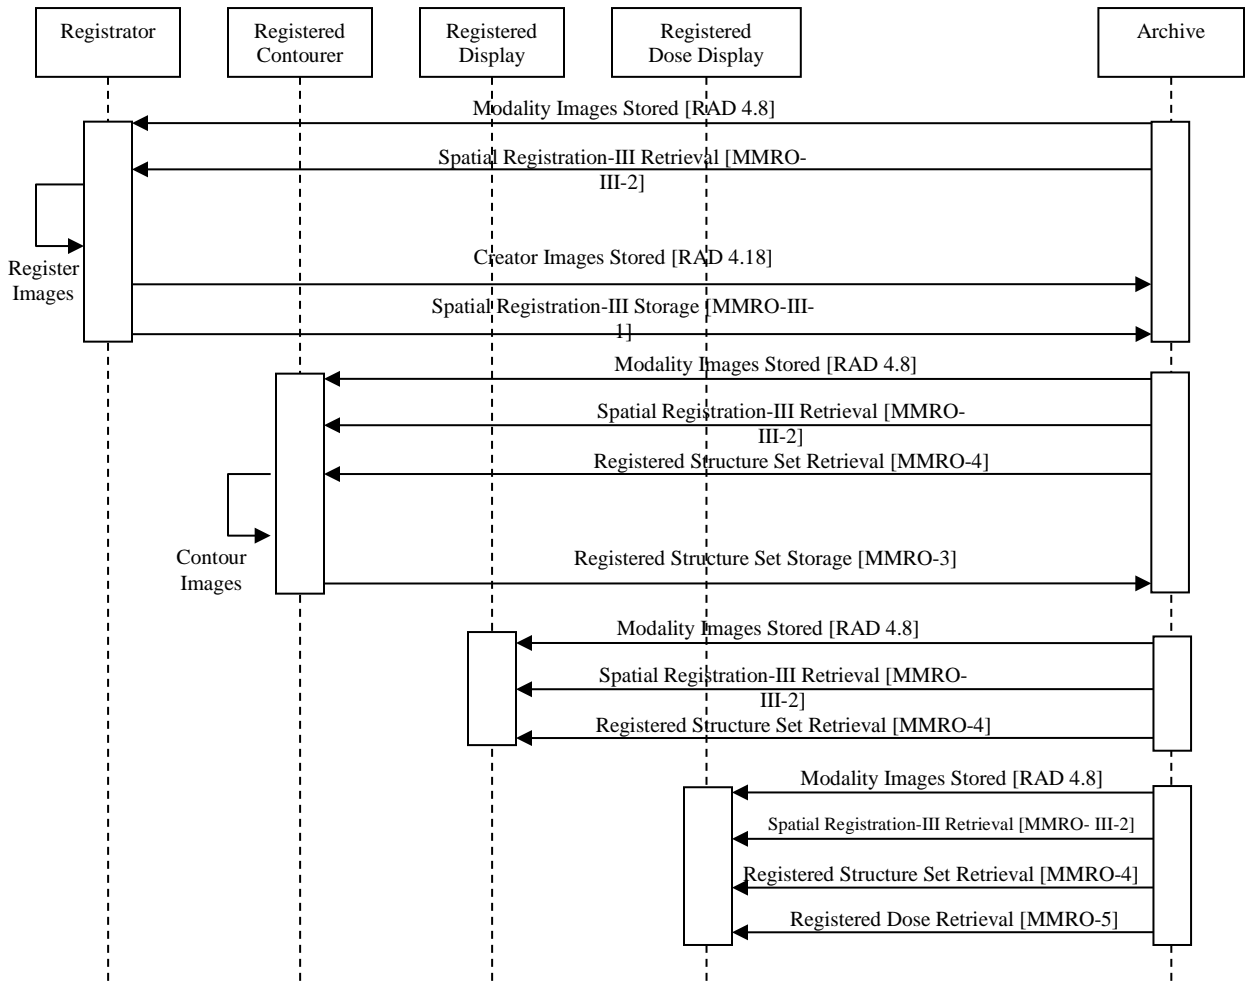

**Figure 4.5-1: Overall Process Flow in MMRO Profile**

### 4.5.1 Concepts

#### 4.5.1.1 Creating Datasets

235 The MMRO-III Profile applies to many types of data. Although each type may need to be handled differently, fused display is possible with each type.

The image sets will usually be created by Acquisition Modality Actors, however in some scenarios the image sets could be the result of post-processing by a Registrator.

240 This profile only addresses the registration of volumetric datasets, RT Structure Set and RT Dose objects.

Volumetric datasets refer to a collection of planar images which span a volume and each image has a defined location in space. Typical examples include a set of CT transverse slices, MR slice stacks and PET transaxial images. In the “easiest” situation, multiple volumetric datasets are created in the same Frame Of Reference. Datasets with the same Frame of Reference value are inherently registered and so a registration step is not strictly necessary.

A shared Frame of Reference may be the result of:

- A hybrid scanner such as a PET/CT being used to image the patient.
- A positioning system, such as a fixed head frame, being used to position the patient at the same location and orientation each time for imaging.
- 250 • A single scanner being used to image the patient at several closely spaced time intervals (e.g., gated cardiac or pulmonary imaging).
- A second image set being created by a post-processing step (e.g., tissue enhancement or tumor segmentation) and inheriting the Frame of Reference of the first image set.

255 Note that image sets with a shared Frame of Reference UID implies they are in the same reference coordinate system, but does not guarantee that they overlap. For example, a pelvis series and a head series from the same MR scan may share a Frame of Reference.

More typically, volumetric datasets are each created with a unique Frame Of Reference.

Different Frames of Reference may be the result of:

- Different equipment being used to image the patient
- 260 • The same piece of equipment being used to image the patient at different times
- Different patients/subjects being imaged (as in a comparative study or when patient images are mapped to an atlas for display or analysis)

#### **4.5.1.2 Registering Datasets**

265 To perform registration when datasets do not share a Frame of Reference, it is necessary to define a relationship between them. Even if two datasets do share a Frame of Reference, for example on the basis of assuming no patient motion, or assuming two acquisition systems are perfectly calibrated, it is sometimes still useful to perform a registration based on fiducials, image content or something else.

270 Once the registration is complete, the resulting transformation is recorded in a Spatial Registration object which is typically stored in the study with the image data. The DICOM Spatial Registration object supports rigid registrations (translation, rotation and scaling).

Spatial Registration objects will usually be created by Registrators; however, in some situations a registration object will not be strictly required (if the datasets share the same Frame of Reference).

275 There are many methods/algorithms for registration: matching fiducials that are visible in the datasets, using operator input to help align the data, correlating the information content in the datasets, etc. Specifying a method/algorithm to use to arrive at the transformation is outside the scope of this profile. The specific method/algorithm used may be of interest to the user (especially when several different registrations exist between the same datasets) so it is  
280 recommended that the name and description of the method be recorded in the resulting Spatial Registration Object.

If the application wishes to allow registration of more than 2 volumetric datasets it shall produce multiple Spatial Registration objects. The first Spatial Registration Object shall establish the Registered Frame of Reference for all of the Spatial Registration Objects. Subsequent objects  
285 shall transform a single volumetric dataset into the Registered Frame of Reference.

In some cases, it is conceivable that a Registrar may combine existing registration information without performing a registration process. For example if a registration exists to map dataset A into Frame of Reference C and another registration exists to map dataset B into Frame of Reference C, the Registrar could use those transforms to produce a new set of Spatial  
290 Registration Objects for dataset A and B which transform into a Registered Frame of Reference.

When registering volumetric datasets, the mapping describes the spatial transformation between Frames of Reference. Since the specific images exist in one of those Frames of Reference, they can be mapped to each other.

295 This profile does not address registering datasets which share a common Frame of Reference. If the application wishes to provide this functionality, it should store one or both of the datasets with a new Frame of Reference UID and allow the user to perform the registration with those datasets. This avoids the need to define a non-unity transform from a Frame of Reference to itself. This capability is not required to satisfy this profile.

300 Identifying and obtaining an appropriate matching pair of datasets to register is necessary but is not defined by this profile. IHE ensures that some useful query parameters are available, but in the end, this task is left to the implementer.

#### **4.5.1.3 Resampling Datasets**

305 After a Spatial Registration has been applied, the data in the two datasets is in the same coordinate system, but may still have different pixel resolution, pixel spacing, slice thickness, number of slices, slice positions or even slice orientations. Before display is possible, it is necessary to resample the registered dataset into the Registered Frame of Reference. Also, the Image Orientation and Patient Position of the resampled dataset shall match that of the Base dataset.



310 Note that when resampling values, such as NM and PET counts, which are not normalized to the  
volume represented by the pixel, the resampled pixel value may be quite different from the  
original pixel value. For example, when creating a new image with twice the number of pixels in  
the X and Y directions, 1 pixel in the original data is now 4 pixels in the resampled data, and the  
value of each of the new pixels would be expected to be roughly  $\frac{1}{4}$  of the value of the original  
315 pixel. When resampling values that are not directly linked to the area/volume of the pixel (such  
as Hounsfield units), the new pixels will have values similar to the original pixel (partial volume  
effects notwithstanding).

The exact values produced by resampling also depend on the interpolation algorithm used. The  
specification of such algorithms is outside the scope of this profile.

320 In the Radiotherapy domain, there will also be instances of RT Structure Set and RT Dose  
objects which exist in the same Frame of Reference as one of the datasets being registered. The  
structures described as contours in the RT Structure Sets will be subject to resampling prior to  
display. The resampling of the contours depends on the resampling algorithm used and is outside  
the scope of this profile.

Resampling of RT Dose objects is not supported within this profile.

325 The Registered Display is required to be able to perform any resampling needed for the display.  
Some Modalities or Registrators may choose to generate resampled datasets. The advantage is  
that such datasets might be useful to non-registration aware display stations, and even when  
provided to IHE Registered Displays, might conceivably provide improved display performance.  
In most cases, however, storing the resampled data will significantly increase bandwidth and  
330 storage costs. This capability is not required to satisfy this profile.

Note that the stepping interval when scrolling through slices may be of primary importance to  
users and care should be taken in that respect. Sometimes the user may wish to step in  
increments of the original slices of the underlying set, and sometimes in the increments of the  
original slice or pixel spacing of the superimposed data set.

#### 335 **4.5.1.4 Presenting Registered Datasets**

Presentation of the Registered Datasets is performed by the Registered Display.

340 No DICOM Query transaction for Spatial Registration objects exists currently. For the purpose  
of this profile, it will be assumed that the registered images and the required Spatial Registration  
objects will be made available to the Registered Display. The data will be transferred via C-  
STORE operations, but the initiation of the action is out of band for this profile.

The Registered Display transforms the datasets by applying the spatial registrations according to  
the DICOM specification, and resamples the datasets as necessary for display.

345 Simple registered display could involve presentation of a single frame at a time. For some  
clinical interpretation tasks, presentation of a registered MPR (Multi Planar Reconstructed) view  
is considered essential. Many users will also expect to be able to change the transparency of the  
fusion overlay (blending factor), the color map for the overlay, the Window Width/Level for

each data set, and other display parameters. For PET data, controls for upper & lower Window Level are valuable.

#### **4.5.1.5 Spatial Registrations and Frame of Reference**

350 This profile requires the Spatial Registration object not only to contain the Frame of References that are registered, but also registered instances (e.g., images). This is required for safety when registering two frames of references without further capability of verification. As an example, there are scanners that acquire two sequential image series, both with the same Frame of Reference. If the patient moves between image acquisitions, there will exist two image series  
355 with the same Frame of Reference, but spatially inconsistent image information.

Applications are required to warn users if they receive Spatial Registration objects without image references. Similarly, warnings should occur if the displayed image sets include images not explicitly listed in the Spatial Registration objects.

#### **4.5.1.6 Well-known Frame of Reference**

360 This profile defines the content and usage of Registrations between image series. Registering image series to a Well-known Frame of Reference is possible, but out of scope of this profile.

Note that when registering multiple image series to a Well-known FOR, ambiguities may occur due to the transitive nature.

### **4.5.2 Use Case #1: Multimodality Contouring**

365 Two or more series of images, for example, CT, MR and PET, are acquired and stored to an archive system. The images, potentially with different Frames of Reference, are read in, registered, and then used for identifying volumes of interest (VOI) which are stored using an RT Structure Set object.

#### **4.5.2.1 Multimodality Contouring Use Case Description**


- 370
- Two or more series of images, for example a CT, MR and PET series, are acquired and reconstructed on multiple different Acquisition Modalities.
  - The image sets, each with a different Frame of Reference, are stored to the Archive.
  - Contrary to prior definitions of this profile, the actors defined here do not require establishing a Registered Frame of Reference which is the Frame of Reference of a CT image series. For  
375 example, to describe the registration of all 3 image sets, 2 Spatial Registration objects will be required. The first may register the CT to the MR, and the second may register the PET to the MR. A Registrator shall be able to accept any combination of Spatial Registration objects and may then internally re-organize the registrations. Any registrations created by a Registrator shall reflect the registrations that were actually performed by the user.
- 380
- A Registered Contourer receives the image sets and Spatial Registrations and creates an RT Structure Set in the same Frame of Reference as one of the datasets. If the image sets are a

superset of the images listed in the Spatial Registration IOD, the application shall warn the user of the use of potentially non-registered images. Each dataset may have a RT Structure Set created in its Frame of Reference.

385 Note that in case structures are resampled from one image set to another, it is currently not possible to indicate where the structures originated.

- The Registered Contourer will store the RT Structure Set(s) to the Archive.
- To render the display, the Registered Display uses the transformation in the Spatial Registration to translate the superimposed data into the same space as the underlying image data. Since each RT Structure Set shares a Frame of Reference UID with one of the datasets, 390 the structures can be transformed by resampling using the same transformation for the volume of interest as defined for the underlying image set.
- The appearance of the fused display is out of band for this profile.

### 4.5.2.2 Multimodality Contouring Process Flow

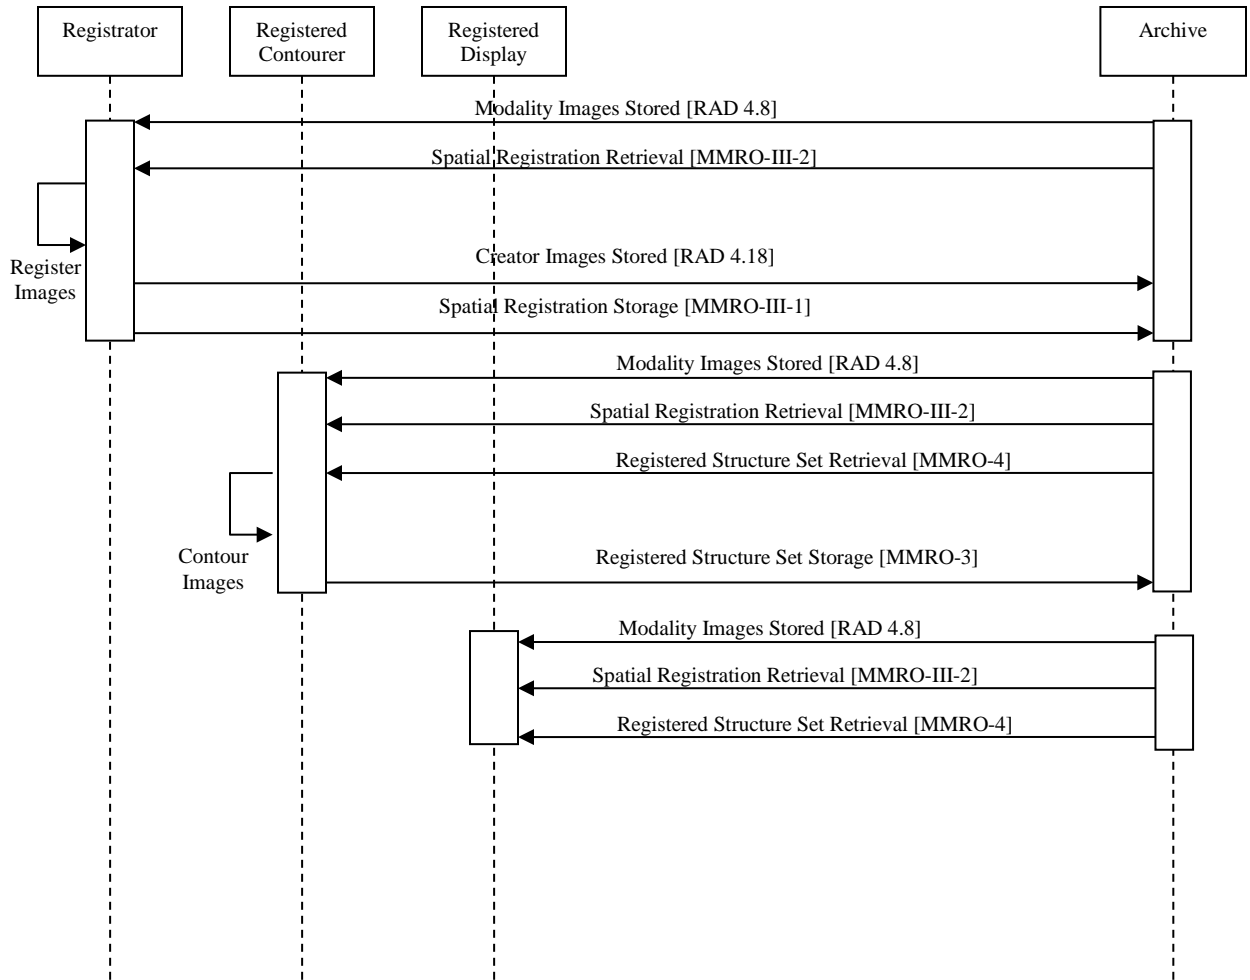

395

Figure 4.5.2.2-1: Process Flow for Multimodality Contouring Use Case

### 4.5.3 Use Case #2: Shared Frame of Reference


Hybrid Modalities, (e.g., PET/CT Scanner) combine two modalities into a single system. Typically, they calibrate the couch motion and scan space and, assuming the patient does not move, store two image sets mapped into a common space (described by a single Frame of Reference). This also applies to RT objects, such as RT Structure Set and RT Dose objects, as they will share a common Frame of Reference with an image set.

400

#### 4.5.3.1 Shared Frame of Reference Use Case Description

- 405
- Two series of images, for example a PET series and a CT series, are acquired and reconstructed on a single hybrid system.
  - The image sets, each with the same Frame of Reference, are stored to the Archive. A common Frame of Reference implies that the two image sets are already in the same coordinate system and no transformation is required.
- 410
- A Registered Contourer retrieves the image sets and creates RT Structure Sets in the same Frame of Reference as the image sets. Each RT Structure Set shall reference only a single image set. If structures are defined for both image sets, two RT Structure Set instances will be created.
  - The Registered Contourer will store the RT Structure Set(s) to the Archive.
- 415
- However, if the patient moves between scans, the shared Frame of Reference does not correctly identify that related pixel information of the separate image datasets are in the same spatial location. Verification and /or an additional registration step is recommended to verify/ensure the correct relation. See also 4.5.1.2 and 4.5.1.5.
- 420
- A Registered Display is sent the image sets and RT Structure Set(s), and observes that no Spatial Registration object is referenced. It also observes that the two image sets and the RT Structure Set share the same Frame of Reference.
  - The Registered Display re-samples the image sets, if necessary to match resolutions for display. No spatial registration transformation is required.
  - The appearance of the fused display is out of band for this profile.

425 **4.5.3.2 Shared Frame of Reference Process Flow**

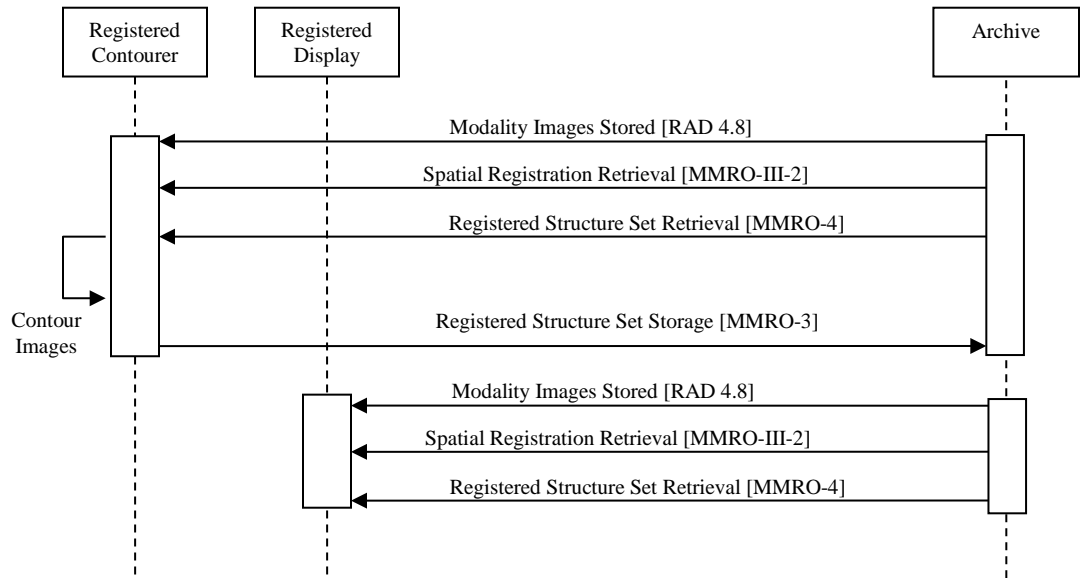

**Figure 4.5.3.2-1: Process Flow for Shared Frame of Reference Use Case**

430 **4.5.4 Use Case #3: Multimodality Dose Display**

Two or more series of images, for example, CT, MR and PET, are acquired and stored to an archive system. The images, potentially with different Frames of Reference, are read in, registered, and then used for identifying volumes of interest (VOI) which are stored using an RT Structure Set object. An RT Dose object is created (out of band) utilizing the information and stored in the Frame of Reference of one of the image sets.

435

**4.5.4.1 Multimodality Dose Display Use Case Description**

- Two or more series of images, for example a CT, MR and PET series, are acquired and reconstructed on multiple different Acquisition Modalities.
- The image sets, each with a different Frame of Reference, are stored to the Archive.
- A treatment plan is created from the image sets, along with RT Structure Sets, an RT Dosimetric Plan, and an RT Dose object.
- A Registered Dose Display is sent the image sets, RT Structure Set(s) and RT Dose along with the required Spatial Registrations.

440

- 445
- The Registered Dose Display re-samples the image sets, RT Structure Sets, and RT Dose as needed for appropriate display.
  - The appearance of the fused display is out of band for this profile.

#### 4.5.4.2 Multimodality Dose Display Process Flow

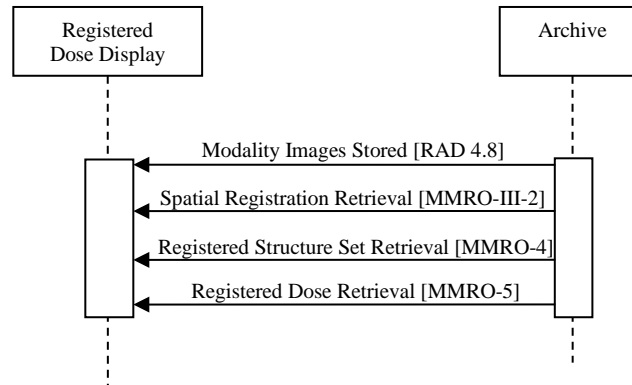


Figure 4.5.4.2-1: Process Flow for Multimodality Dose Display Use Case

450

## 4.6 MMRO-III Security Considerations

No specific considerations.

## 4.7 MMRO-III Cross Profile Considerations

No specific considerations.

455

# Appendices

## Actor Summary Definitions

*Add the following terms to the IHE TF General Introduction Namespace list of actors:*

460 No new definitions.

## Transaction Summary Definitions

*Add the following terms to the IHE TF General Introduction Namespace list of transactions:*

### MMRO-III-1: Spatial Registration Storage

465 In the Spatial Registration Storage transaction, the **Registrar** stores one or more Spatial Registration instances to the **Archive**. Spatial registration objects define how the pixel coordinates of one image data set are transformed to another coordinate system (for example to a coordinate system defined by another image data set thus allowing each dataset to be spatially aligned). A list of the images used in each Frame of Reference to determine the spatial registration shall be stored in the Spatial Registration instance.

470

### MMRO-III-2: Spatial Registration Retrieval

A **Registered Display**, **Registered Dose Display** or **Registered Contourer** receives from an **Archive** one or more Spatial Registration objects carrying the transformation information to be applied to two image data sets intended for further processing or registered display. Each application receiving a Spatial Registration instance shall compare the image set to be used / displayed to the list of images for each Frame of Reference and warn the user if additional images are to be displayed for which the spatial registration may not be defined.

475



## **Glossary**

480

*Add the following terms to the IHE Technical Frameworks General Introduction Glossary:*

## **Volume 2 – Transactions**

### 3 Transactions

Add the following to Section 3


#### 3.14 MMRO-3: Registered Structure Set Storage

485 This section corresponds to Transaction MMRO-3 of the IHE-RO Technical Framework. Transaction MMRO-3 is used by the *Registered Contourer* and *Archive* Actors.

##### 3.14.1 Scope

In the Registered Structure Set Storage Transaction, the Registered Contourer stores a Structure Set on an Archive to make it available.

490 **3.14.2 Use Case Roles**

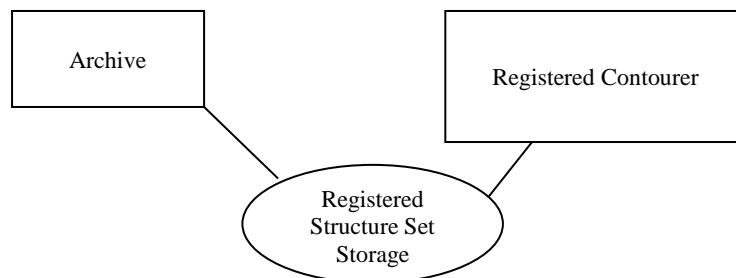


<b>Actor:</b>	Archive
<b>Role:</b>	Receive and store a Structure Set instance from the <i>Registered Contourer</i>
<b>Actor:</b>	Registered Contourer
<b>Role:</b>	Send a Structure Set instance for storage

##### 3.14.3 Referenced standards

DICOM 2007 PS3.4: Storage Service Class

DICOM 2007 PS 3.4: RT Structure Set Storage

495 **3.14.4 Interaction Diagram**

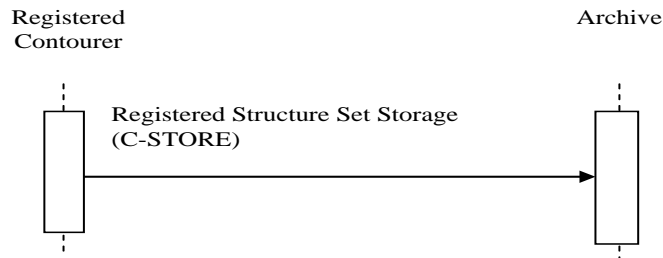

**3.14.4.1 Registered Structure Set Storage**

**3.14.4.1.1 Trigger Events**

The user of the Registered Contourer selects a one or more Structure Sets to store.

500 **3.14.1.1.1 Message Semantics**

The message semantics are defined by the DICOM Storage SOP Class. The Registered Contourer is the storage SCU and the Archive is the storage SCP.

505 The Contours in the ROI Contour module are restricted to Geometric Type POINT and CLOSED\_PLANAR. ROI contours must correspond to exported image plane locations. If a system does not support unequally-spaced slices, for example, that system is responsible for creating a resampled image set (see RO-11) and creating a structure set in which the ROI contours reference the resampled image set. Absence of an ROI contour on a slice between slices on which contours are defined implies that the ROI does not intersect that slice.

510 An RT Structure Set object generated by a Registered Contourer will reference images from a single series and share the Frame of Reference UID of that series. It is implied that the coordinates in that object will exist in the coordinate system identified by the FoR UID. Finally, contours will exist on the same plane as the referenced image slices.

515 To make ROI's available to the downstream planning process or to the 2007 Basic RT Objects Interoperability Profile's Contourer, the Registrator shall be able not only to transform contours from a source Frame of Reference to the Registered Frame of Reference, but also to resample the contour to the planes of the images referenced in the RT Structure Set which corresponds to the Registered Frame of Reference.

520 The set of contours transmitted in an RT Structure Set must not assume interpolation of contours across image slices. Absence of an ROI contour on a slice between slices on which contours are defined implies that the ROI does not intersect that slice.

The MMRO Profile has implicit limitations imposed by its dependency on the IHE-RO BRTO Profile. These limitations are described in the MMRO Profile description in Volume 1 of the IHE-RO Technical Frameworks.

525 Also, refer to appendix B for an overview of the specific requirements on the DICOM attributes that are included in an RT Structure Set object. In particular, the structure set must share a single frame of reference UID with the images.

### 3.14.1.1.2 Expected Actions

Upon receipt of the Structure Set, the Archive shall store it. This Structure Set is then available for subsequent retrieval (RO-7 and MMRO-4).

## 530 3.14.5 Security Considerations

### 3.14.5.1 Security Audit Considerations

#### 3.14.5.1.1 Actor Specific Security Considerations


## 3.15 MMRO-4: Registered Structure Set Retrieval

535 This section corresponds to Transaction MMRO-4 of the IHE-RO Technical *Framework*. *Transaction MMRO-4 is used by the Registered Contourer, Registered Display, Registered Dose Display, and Archive* Actors.

### 3.15.1 Scope

In the Registered Structure Set Retrieval Transaction, the *Archive* stores a Structure Set on a *Registered Contourer, Registered Display or Registered Dose Display*.

## 540 3.15.2 Use Case Roles

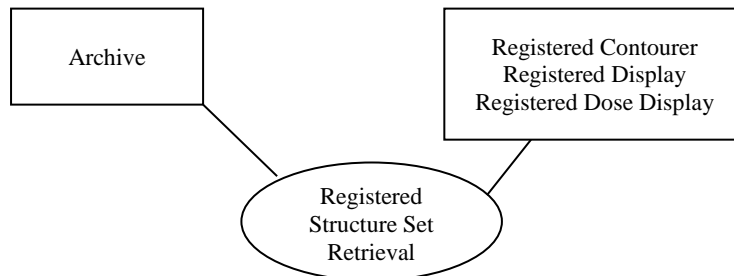

<b>Actor:</b>	Archive
<b>Role:</b>	Send Registered Structure Set instance(s) to the receiving actor
<b>Actor:</b>	Registered Contourer, Registered Display, Registered Dose Display


<b>Role:</b>	Receive Registered Structure Set instances from the <i>Archive</i>
--------------	--

### 3.15.3 Referenced standards

DICOM 2007 PS3.4: Storage Service Class

DICOM 2007 PS 3.4: RT Structure Set Storage

### 545 3.15.4 Interaction Diagram

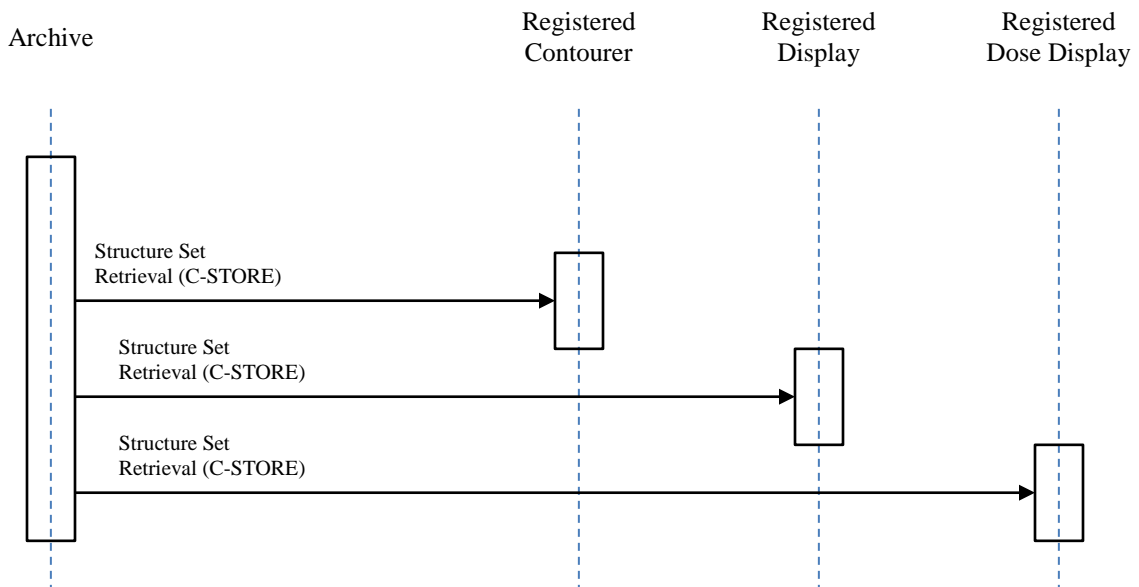

#### 3.15.4.1 Registered Structure Set Retrieval

##### 3.15.4.1.1 Trigger Events

550 The user of the *Registered Contourer* determines that a new set of contours is to be based upon an existing Structure Set, and requests that the *Archive* send this Structure Set to the *Registered Contourer*.

The user of the *Registered Display* determines that a display is to be based upon an existing Structure Set, and requests that the *Archive* send this Structure Set to the *Registered Display*.

555 The user of the *Registered Dose Display* determines that a dose display is to be based upon an existing Structure Set, and requests that the *Archive* send this Structure Set to the *Registered Dose Display*.

The mechanism(s) by which these transfers are initiated is outside the scope of this profile.

### 3.15.4.1.2 Message Semantics

560 The message semantics are defined by the DICOM Storage SOP Class. The *Registered Contourer*, *Registered Display* or *Registered Dose Display* is the storage SCP and the *Archive* is the storage SCU.

Absence of an ROI contour on a slice between slices on which contours are defined implies that the ROI does not intersect that slice.

565 Also, refer to appendix B for an overview of the specific requirements on the DICOM attributes that are included in an RT Structure Set object. In particular, the structure set must have the same study instance UID, but a different series instance UID, than the CT image series upon which the contours are based.

### 3.15.4.1.3 Expected Actions

570 The *Registered Contourer* will upload image data sets, related structure sets and spatial registration objects. It will present the user with a *Registered Display*, and allow the user to then construct a new set of contours which will later be exported as a new structure set (MMRO-3: Registered Structure Set Storage). The new structure set will have the same Frame of Reference UID and Study Instance UID of the original base image data set and structure set.

575 The *Registered Display* will load image data sets, related structure sets and spatial registration objects. It will display the information to the user.

The *Registered Dose Display* will load image data sets, related structure sets, dose and spatial registration objects. It will display the information to the user.

580 The *Registered Contourer* will load all of the Structure Set, and will relate it to images based on the Frame of Reference UID. The contours contained will then be available to the user of the *Registered Contourer* for use in construction a new set of contours which will later be exported as a structure set (MMRO-3: Registered Structure Set Storage). This new structure set will have the same frame of reference UID and study instance UID of the original images and structure set.

## 3.15.5 Security Considerations

### 3.15.5.1 Security Audit Considerations

585 3.15.5.1.1 Actor Specific Security Considerations


## 3.16 MMRO-5: Registered Dose Retrieval

This section corresponds to MMRO-5 of the IHE-RO technical framework. Transaction MMRO-5 is used by the *Archive* and *Registered Dose Display*.

### 3.16.1 Scope

590 In the Registered Dose Retrieval Transaction, the requested RT Dose is transferred from the *Archive* to the *Registered Dose Display*.

### 3.16.2 Use Case Roles

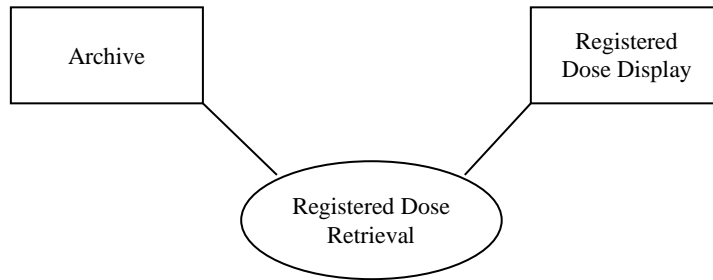


<b>Actor:</b>	Archive
<b>Role:</b>	Sends Registered Dose instance to the <i>Registered Dose Display</i>
<b>Actor:</b>	Registered Dose Display
<b>Role:</b>	Receives the Registered Dose instance from the <i>Archive</i>

### 3.16.3 Referenced Standards

- 595 DICOM 2007 PS3.4: Storage Service Class
- DICOM 2007 PS 3.4: RT Dose Storage

### 3.16.4 Interaction Diagram

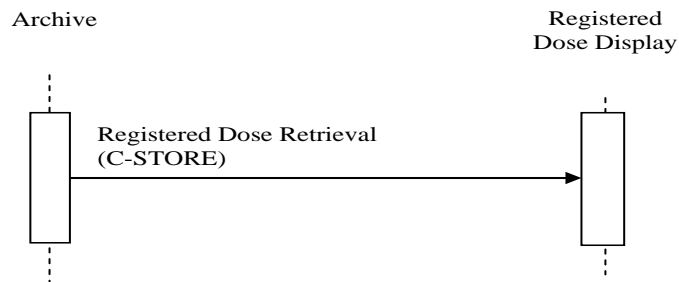

#### 3.16.4.1 Registered Dose Retrieval

##### 600 3.16.4.1.1 Trigger Events

The user of the *Registered Dose Display* selects an RT Dose instance for display in the context of a one or more CT Image Sets and the targets and avoidance structures defined by corresponding RT Structure Set.



### 3.16.4.1.2 Message Semantics

605 The *Archive* uses the DICOM C-STORE message to transfer the dose. The *Archive* is the DICOM Storage SCU and the *Registered Dose Display* is the DICOM Storage SCP.

This transaction shall support Dose represented as a three-dimensional dose array sampled onto axial image planes in the same DICOM Patient coordinate system Frame of Reference as the diagnostic images used to compute it. The dose image shall be orthogonal with respect to the  
610 DICOM patient coordinate system: the value of Image Orientation (Patient) (0020,0037) shall be  $[\pm 1, 0, 0, 0, \pm 1, 0]$ , within an uncertainty of 0.001 Radians. Dose Planes may be irregularly spaced, and they need not correspond to image planes.

Not supported are point doses, projection of dose onto an oblique plane, iso-dose contours and dose-volume histograms. The dose pixels shall represent absolute physical dose in units of Gray.  
615 The value of Dose Units (3004,0002) shall be GY. The value of Pixel Representation (0016,0103) shall be 0; negative dose values shall not be present.

The RT Dose shall always share the same Frame of Reference as the related RT Plan.

### 3.16.4.1.3 Expected Actions

Upon receiving the request for retrieval, the *Archive* shall return the requested RT Dose to the  
620 *Registered Dose Display*. The *Registered Dose Display* shall validate the received RT Dose. If the received RT Dose is valid, it shall be loaded in the *Registered Dose Display*. If it is not valid, a warning message shall be displayed to the user, indicating the reason why it is not valid.

The received Dose will be displayed in the same coordinate system as the image set on which it was computed.

## 625 3.16.5 Security Considerations

### 3.16.5.1 Security Audit Considerations

#### 3.16.5.1.1 Actor Specific Security Considerations


## 3.17 MMRO-III-1: Spatial Registration-III Storage

This section corresponds to the Spatial Registration-III Storage transaction of the IHE-RO  
630 Technical Framework. Transaction MMRO-II-1 is used by the *Archive* and *Registrar* Actors.

### 3.17.1 Scope

In the Spatial Registration-III Storage transaction, the *Registrar* sends one or more Spatial Registration instances to the *Archive*. Spatial registration objects define how the pixel coordinates of one image data set are transformed to another coordinate system (for example to a  
635 coordinate system defined by another image data set thus allowing each dataset to be spatially aligned).

### 3.17.2 Use Case Roles

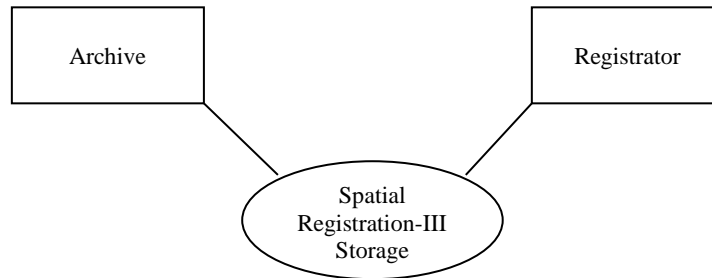


<b>Actor:</b>	Archive
<b>Role:</b>	Accept and store Spatial Registration instances from <i>Registrator</i> Actors
<b>Actor:</b>	Registrator
<b>Role:</b>	Create and transmit Spatial Registration instances to an <i>Archive</i>

### 3.17.3 Referenced Standards

- 640 DICOM 2011 PS 3.4: Storage Service Class
- DICOM 2011 PS 3.4: Spatial Registration Storage

### 3.17.4 Interaction Diagram

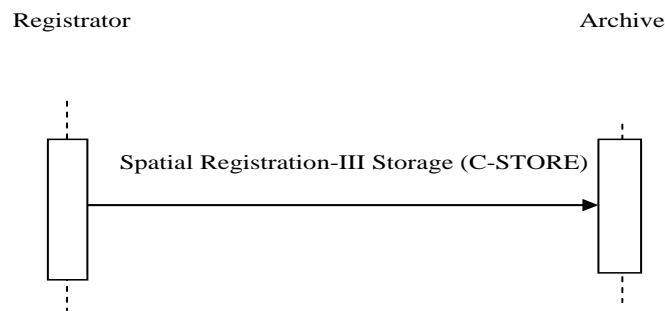

#### 3.17.4.1 Spatial Registration-III Storage

##### 645 3.17.4.1.1 Trigger Events

A *Registrator* chooses to transfer one or more Spatial Registration objects to the *Archive*. This may follow creation of the Spatial Registration object as part of a registration process.

### 3.17.4.1.2 Message Semantics

650 The **Registrar** uses the DICOM C-STORE message to transfer the Spatial Registration objects. The **Registrar** acts in the role of the DICOM Storage SCU and the **Archive** is the DICOM Storage SCP.

The **Registrar** is responsible for warning the user of mismatched patient demographics within registered series.

655 The Spatial Registration shall contain two Registration Sequences. Refer to DICOM 2011 PS 3.17 Figure O.4-1 for informative details on the structure of the Registration Sequences.

660 When registering volumetric datasets with different Frames of Reference, each Registration Sequence shall define the transformation of the corresponding Original Dataset into the Registered Frame of Reference. Typically, one of the Registration Sequences will contain an IDENTITY transform, indicating that the corresponding original dataset established the Registered Frame of Reference. In that case, the Frame of Reference of the Spatial Registration object may be the same as the Frame of Reference of that Original Dataset.

665 When registering more than 2 Frames of Reference each Spatial Registration object shall include a reference to the Registered Frame of Reference UID with an IDENTITY transformation as one of the elements of the Registration Sequence. Each Spatial Registration object shall specify its Frame of Reference UID attribute to be the same as the Registered Frame of Reference UID.

This profile shall not allow the re-registration of multiple series with the same Frame of Reference. The actor may re-write one or both of the series with new Frames of Reference and perform the registration on the new series. This capability is not required to satisfy this transaction.

670 A Registration Sequence item shall contain a Frame of Reference and a list of images which have been available to the user at the time of definition and contributed to the definition of the spatial registration. Images not included in the list of images shall not be assumed to be consistent with the Spatial Registration recorded, e.g., registration of these images is unverified.

675 Contrary to prior versions of this profile, the MMRO-III Profile does not have any implicit limitations: there is no requirement to specify a “base” or “primary” image set that is a CT. There is also no limitation that registrations shall be performed to a specific “base” or “primary” image set.

Modifying an existing Spatial Registration Object shall result in a new instance with a new instance UID.

680 The Spatial Registration object shall be stored:

- in the Study to which the Registered Frame of Reference belongs. This Study is identified by the Study UID of the images which establish the Registered Frame of Reference in the Spatial Registration objects as described above.
- in a different series from images.

685 **3.17.4.1.3 Expected Actions**

The Archive will store the received Spatial Registration objects. The Spatial Registration objects shall be stored such that they can be later retrieved (See MMRO-III-2 Spatial Registration Retrieval) in a fashion meeting the requirements defined for a DICOM Level 2 Storage SCP (see DICOM PS 3.4 B.4.1).

690 **3.17.5 Security Considerations**

**3.17.5.1 Security Audit Considerations**

**3.17.5.1.1 Actor Specific Security Considerations**


**3.18 MMRO-III-2: Spatial Registration-III Retrieval**

695 This section corresponds to Transaction MMRO-III-2 of the IHE-RO Technical Framework. Transaction MMRO-III-2 is used by the *Registered Contourer*, *Registered Display*, *Registered Dose Display* and *Archive* Actors. It is optionally used by the *Registrar*.

**3.18.1 Scope**

700 A *Registered Contourer*, *Registered Display* or *Registered Dose Display* receives from an *Archive* one or more Spatial Registration objects carrying the transformation information to be applied to two image data sets intended for further processing or fused display. A *Registrar* may (optional transaction) receive from an *Archive* one or more Spatial Registration objects.

**3.18.2 Use Case Roles**

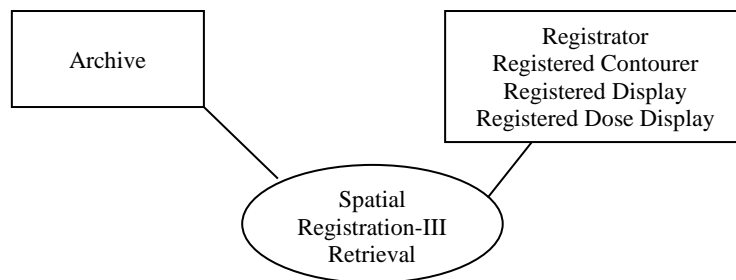


<b>Actor:</b>	Archive
<b>Role:</b>	Send Spatial Registration instance(s) to the receiving actor
<b>Actor:</b>	Registered Contourer, Registered Display, Registered Dose Display
<b>Role:</b>	Receive Spatial Registration instances from the <i>Archive</i>

<b>Actor:</b>	Registrator (optional)
<b>Role:</b>	Receive Spatial Registration instances from the <i>Archive</i>

### 3.18.3 Referenced Standards

- 705 DICOM 2011 PS 3.4: Storage Service Class
- DICOM 2011 PS 3.4: CT Image Storage
- DICOM 2011 PS 3.4: MR Image Storage
- DICOM 2011 PS 3.4: Positron Emission Tomography Image Storage
- DICOM 2011 PS 3.4: Spatial Registration Storage

### 710 3.18.4 Interaction Diagram

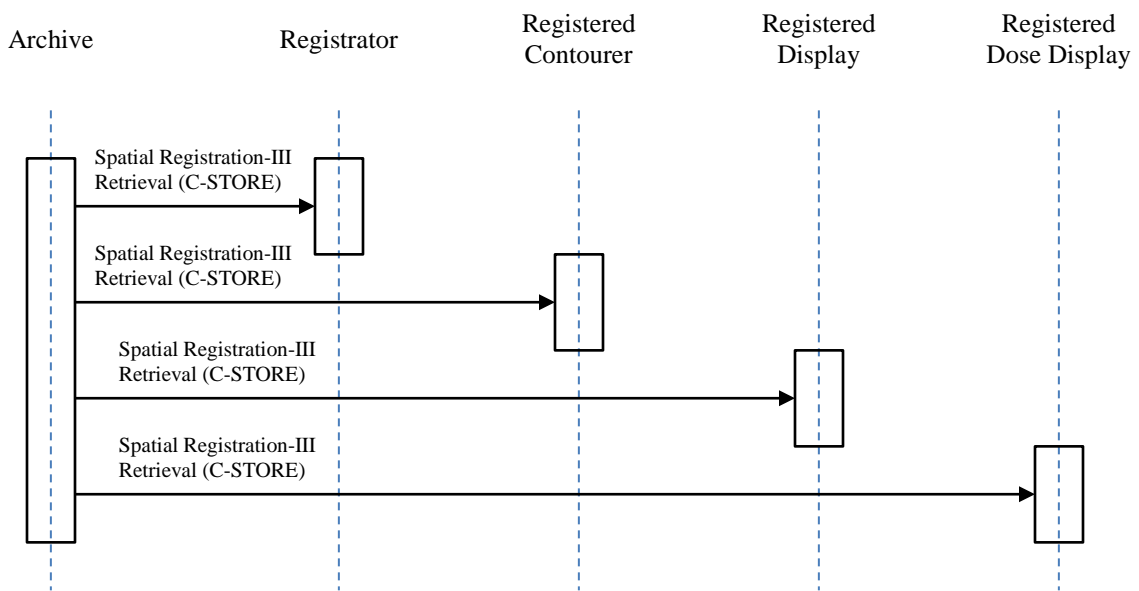

#### 3.18.4.1 Spatial Registration-II Storage

##### 3.18.4.1.1 Trigger Events

715 The *Registered Contourer*, *Registered Display*, *Registered Dose Display* or (optionally) *Registrator* receives one or more specific Spatial Registration objects from the *Archive*.

### 3.18.4.1.2 Message Semantics

The *Archive* uses the DICOM C-STORE message to transfer the Spatial Registration objects. The *Registered Contourer*, *Registered Display* or *Registered Dose Display* is the DICOM Storage SCU and the *Archive* is the DICOM Storage SCP.

720 It is the responsibility of the *Registered Contourer*, *Registered Display* or *Registered Dose Display* to apply the Spatial Registration as defined in DICOM. Refer to DICOM 2011 PS 3.4, Annex C, for detailed descriptive semantics.

725 It is the responsibility of the *Registered Contourer*, *Registered Display* or *Registered Dose Display* to verify that the Registration Sequence item in the Spatial Registration contains a Frame of Reference and a list of images. Image instances present but not included in the list of images shall not be assumed to be consistent with the Spatial Registration recorded, e.g., registration of these images is unverified.

The *Registered Contourer*, *Registered Display* or *Registered Dose Display* may want to re-organize the order and direction of Registrations accordingly.

### 730 3.18.4.1.3 Expected Actions

The *Archive* establishes a DICOM association with the *Registered Contourer*, *Registered Display* or *Registered Dose Display*, and uses the DICOM Spatial Registration Storage SOP Class to transfer the requested Spatial Registration objects.

735 The *Registered Contourer*, *Registered Display* or *Registered Dose Display* shall use the most recently received instances to ensure that the most recent patient data from the Archive is displayed.

## 3.18.5 Security Considerations

### 3.18.5.1 Security Audit Considerations

#### 3.18.5.1.1 Actor Specific Security Considerations

740

## Appendix A – Attribute Consistency between Composite IODs

### A.1 Radiation Oncology Critical Attribute Mapping

*Add the 2<sup>nd</sup> column of the following table to Table A.1-1 structure*

Attribute (Tag)	Spatial Registration
Patient's Name (0010,0010)	Copy
Patient ID (0010,0020)	Copy
Patient's Birth Date (0010,0030)	Copy
Patient's Sex (0010,0040)	Copy
Study Instance UID (0020,000D)	Copy from Base Study Images **
Study Date (0008,0020)	Copy from Base Study Images **
Study Time (0008,0030)	Copy from Base Study Images **
Referring Physician's Name (0008,0090)	Copy from Base Study Images **
Study ID (0020,0010)	Copy from Base Study Images **
Accession Number (0008,0050)	Copy from Base Study Images **
Study Description (0008,1030)	Copy from Base Study Images **
Frame of Reference UID (0020,0052)	Copy from Base Study Images **
Position Reference Indicator (0020,1040)	Copy from Base Study Images **

745

\*\* The Base Study Images are identified as the images which establish the Registered Frame of Reference of the Spatial Registration objects.

### A.2 Radiation Oncology Critical Modules

*Add the following at the end of Appendix A.2*

750 Table A.2-3 describes requirements, recommendations or explanations on integration-critical DICOM modules for radiation oncology cases. It defines which integration-critical modules need to be populated for the Spatial Registration IOD. The table follows the structure defined in DICOM PS3.3 Section A.1.3.

755 **Table A.2-3: Spatial Registration IOD Modules**

IE	Module	Reference	Usage	IHE-RO Usage
Patient	Patient	C.7.1.1	M	M
	Clinical Trial Subject	C.7.1.3	U	U
Study	General Study	C.7.2.1	M	M
	Patient Study	C.7.2.2	U	U
	Clinical Trial Study	C.7.2.3	U	U
Series	General Series	C.7.3.1	M	M
	Clinical Trial Series	C.7.3.2	U	U
	Spatial Registration Series	C.20.1	M	M
Frame of Reference	Frame of Reference	C.7.4.1	M	M
Equipment	General Equipment	C.7.5.1	M	M
Spatial Registration	Spatial Registration	C.20.2	M	M
	Common Instance Reference	C.12.2	M	M
	SOP Common	C.12.1	M	M

### A.3 Radiation Oncology Critical Attributes

*Edit the tables in A.3 per the instructions below:*

760 *The following tables lists redefinitions of attributes within the Multimodality Image Registration for Radiation Oncology Integration Profile, which have already been defined in other integration profiles. Attributes displayed in a light grey value are not modified but only added to provide the context in which a certain attribute enhancement is defined.*

**Table A.3-12: Structure Set Module Attributes**

Attribute	Tag	Type	Attribute Note
Structure Set Label	(3006,0002)	R+	
Structure Set Date	(3006,0008)	R+	
Structure Set Time	(3006,0009)	R+	



IHE Radiation Oncology Technical Framework Supplement – Multimodality Image Registration for Radiation Oncology 2013 (MMRO-III)

Attribute	Tag	Type	Attribute Note
Referenced Frame of Reference Sequence	(3006,0010)	R+*	This element is required for all 3D RT Structure Sets which are image based. It is to contain a set of references to the entire set of images which comprise the volume from which the Structure Set was constructed, and which is to be used for planning. There should only be one item in this sequence, as a BRTO Profile-based structure is based on a single set of images, which are all in the same frame of reference.
>Frame of Reference UID	(0020,0052)	R+*	This frame of reference UID shall be the same as the frame of reference of the CT series from which the Structure Set was constructed. It will also be the same as the frame of reference of any related RTPLAN's or RTDOSE's.
>RT Referenced Study Sequence	(3006,0012)	R+*	Shall be present and contain the series sequence. Only one item allowed in this sequence.
>>Referenced SOP Instance UID	(0008,1155)	R+*	This Study Instance UID shall be the same as the Study Instance UID of the related CT instances.
>>RT Referenced Series Sequence	(3006,0014)	R+*	Shall be present to contain the Contour Image Sequence. Only one item allowed in this sequence.
>>>Series Instance UID	(0020,000E)	R+*	Shall be present and contain the series to which the set of CT images upon which the structure set is based belong.
>>>Contour Image Sequence	(3006,0016)	R+*	Shall be present. Contains an item for each CT image in the volume upon which the Structure Set is based.
>>>>Referenced SOP Class UID	(0008,1155)	R+*	<b>Must be present with a value of enhancement '1.2.840.10008.5.1.4.1.1.2', '1.2.840.10008.5.1.4.1.1.4' or '1.2.840.10008.5.1.4.1.1.128'</b>
>>>>Referenced Frame Number	(0008,1160)	O+*	Shall not be present
Structure Set ROI Sequence	(3006,0020)	R+*	This sequence shall be present. It defines the ROI's in this Structure Set.
>ROI Number	(3006,0022)	R*	This defines an index to be used for referencing a particular ROI item from other sequences. It is required to be unique within the Structure Set in which it is created. No limitation on values other than uniqueness within sequence.
>Referenced Frame of Reference UID	(3006,0024)	R*	This frame of reference UID shall be the same as the frame of reference UID of the CT series from which the Structure Set was constructed. It will also be the same as the frame of reference of any related RTPLAN or RTDOSE instances.
>ROI Name	(3006,0026)	R+	This is the primary identifier for an ROI (from user perspective). Shall be present and should match UI display. Shall be unique within the Structure Set ROI sequence.
>ROI Description	(3006,0028)	O+*	Not required - no compliant implementation shall rely on this element being present for proper operation.
>ROI Volume	(3006,002C)	O+*	Not required - no compliant implementation shall rely on this element being present for proper operation.

Attribute	Tag	Type	Attribute Note
>ROI Generation Algorithm	(3006,0036)	R+	<p>Must be present, with a value of AUTOMATIC, SEMIAUTOMATIC, MANUAL, or RESAMPLED. This information may be presented to a user, but no semantics for handling an RTSTRUCT is required for this profile.</p> <p>RESAMPLED indicates that the ROI Contours have been resampled onto a different set of images from those on which the contours were originally created.</p> <p>Implementations which create RTSTRUCT instances must provide an appropriate value.</p>

765

**Table A.3-16: Spatial Registration Module Attributes**

Attribute	Tag	Type	Attribute Note
Registration Sequence	(0070,0308)	R	A sequence of 2 registration items. One Frame of Reference will be to the Registered Frame of Reference, the second will define the spatial registration from the specified Frame of Reference to the Registered Frame of Reference.
>Frame of Reference UID	(0020,0052)	R*	Identifies a Frame of Reference that may or may not be an image set (e.g., atlas or physical space). See C.7.4.1.1.1 for further explanation. Shall be present.
>Referenced Image Sequence	(0008,1140)	R*	Identifies the set of images registered in this sequence item. One or more items shall be present. Represents the set of images available to the Registrator at the time of spatial registration (see Section 3.17.4.1.2).
>>Include 'Image SOP Instance Reference Macro' Table 10-3			
>Matrix Registration Sequence	(0070,0309)	R	A sequence that specifies one spatial registration. Exactly one item shall be present
>>Matrix Sequence	(0070,030A)	R	One item shall be present. The item specifies a transformation. See C.20.2.1.1.
>>>Frame of Reference Transformation Matrix	(3006,00C6)	R	A 4x4 homogeneous transformation matrix that registers the referenced images to the Registered Frame of Reference. Matrix elements shall be listed in row-major order. See C.20.2.1.1.
>>>Frame of Reference Transformation Matrix Type	(0070,030C)	R	The only type of Frame of Reference Transformation Matrix (3006,00C6) supported in this profile is RIGID. See C.20.2.1.2